



Chlorine (Cl₂) or chlorine dioxide (ClO₂) Sensor Cube

- Fully compatible with büS systems and a wide range of further analysis sensor cubes
- Optional pH compensated chlorine measurement
- Modular sensor cube for hot swap (exchange during operation)
- Minimal sample water flow needed
- MEMS technology sensor



Product variants described in the data sheet may differ from the product presentation and description.

Can be combined with

| | |
|---|--|
|  | Type 8905 Online Analysis System ▶ |
|  | Type 8920 Bürkert Communicator ▶ |

Type description

The device is selectable to measure chlorine or chlorine dioxide in water. It is used within the Online Analysis System Type 8905 by being plugged into a spare fluidic backplane slot.

The sensor cube contains a high precision membrane covered amperometric sensor, based on a Bürkert microelectromechanical systems technology (MEMS). The measurement signal shows the Cl₂ or ClO₂ content within the sample water. The chlorine measurement reflects either the available chlorine HOCl or, if coupled with a MS01 pH sensor cube for pH compensation, the free chlorine.

The electrical and fluidic connections are made via the connection panel of the system. The sensor cube is communicating with the system via büS, allowing fully automatic login to the online analysis system. If the sensor is plugged into the system, it automatically logs on to the büS and can be parameterised according to customer requirements.

DTS 1000220807 EN Version: J Status: RL (released | freigegeben | valide) printed: 20.12.2019



Table of contents

| | |
|--|----------|
| 1. General technical data | 3 |
| 2. Materials | 4 |
| 2.1. Chemical Resistance Chart – Bürkert resistApp..... | 4 |
| 3. Dimensions | 5 |
| 4. Product installation | 5 |
| 4.1. Installation notes..... | 5 |
| 5. Product design and assembly | 6 |
| 5.1. Product features | 6 |
| 6. Ordering information | 6 |
| 6.1. Bürkert eShop – Easy ordering and quick delivery..... | 6 |
| 6.2. Bürkert product filter..... | 6 |
| 6.3. Ordering chart..... | 7 |
| 6.4. Ordering chart accessories..... | 7 |

1. General technical data

Product properties

Material

Please make sure the device materials are compatible with the fluid you are using.

Detailed information can be found in chapter **"2.1. Chemical Resistance Chart – Bürkert resistApp"** on page 4.

| | |
|----------------------------------|--|
| Housing | PPE+PS |
| Lever | Zamak, painted |
| Seals | EPDM |
| Dimensions | Detailed information can be found in chapter "3. Dimensions" on page 5. |
| Chlorine/chlorine dioxide sensor | Membrane covered PT-cell, amperometric 3 electrodes measurement, without electrolyte |
| Temperature sensor | Pt1000 Class B, no contact with the water sample |
| Compatibility | With Online Analysis System Type 8905 (the electrical and fluidic contact is made via backplane system.) Detailed information can be found in the data sheet of the online analysis system, see data sheet Type 8905 ▶ for more information. |

Measuring range

| | |
|--|---|
| Chlorine measurement (Cl ₂) | 0.01...5 ppm |
| Chlorine measurement (ClO ₂) | 0.005...5 ppm |
| Maintenance | 12 months nominal, depending on the water quality |

Performance data

Chlorine measurement (Cl₂)

| | |
|----------------------------------|---|
| Sensitivity | - 11 nA/ppm (at pH 5), - 8 nA/ppm (at pH 7) |
| pH compensation | Yes, with MS01 sensor cube Detailed information can be found in the data sheet of the pH sensor cube, see data sheet Type MS01 ▶ for more information |
| Measuring range resolution | 0.01 ppm |
| Measurement deviation | ±0.03 ppm or ± 5 % of the measured value |
| Linearity | ±0.02 ppm of the measured value |
| Repeatability | ±0.02 ppm of the measured value |
| Response time (t ₉₀) | <30 s |

Chlorine measurement (ClO₂)

| | |
|----------------------------------|---|
| Sensitivity | - 4 nA/ppm |
| pH compensation | No |
| Measuring range resolution | 0.001 ppm |
| Measurement deviation | ±0.005 ppm or ± 3 % of the measured value (the greater value applies) |
| Linearity | ±0.01 ppm or ± 3 % of the measured value (the greater value applies) |
| Repeatability | ±0.01 ppm or ± 3 % of the measured value (the greater value applies) |
| Response time (t ₉₀) | <30 s |
| Temperature measurement | 0...+ 50 °C (+32...+ 122 °F) |

Electrical data

| | |
|-------------------|---|
| Operating voltage | 24 V DC through the backplane of the system Type 8905 via büS |
| Power consumption | 0.8 VA |

Media data

| | |
|--------------|---|
| Fluid | Water without particles: drinking water, industrial water |
| pH range | pH 4...pH 9 |
| Conductivity | >50 µs/cm |

Sample water

| | |
|-------------|-----------------------------|
| Temperature | +3...+40 °C (+37...+104 °F) |
| Pressure | PN3 |
| Flow rate | >6 l/h |


Process/Port connection & communication

| | |
|--------------------|---|
| Process connection | Via pinch valve in the fluidic backplane of the Type 8905 Detailed information can be found in the data sheet of the Online Analysis System, see data sheet Type 8905 ▶ for more information. |
|--------------------|---|

| | |
|--|---|
| Electrical connection | Spring contacts in the fluidic backplane of the Type 8905, which is connected to a büS System Detailed information can be found in the data sheet of the Online Analysis System, see data sheet Type 8905 ▶ for more information. |
| Data transfer | |
| Internal communication | Through büS (Bürkert bus, CANopen protocol) |
| External communication by status LED | According to NAMUR NE 107 |
| Approvals and Certificates | |
| Standards | |
| Protection class according to IEC/EN 60529 | <ul style="list-style-type: none"> • IP65, when plugged in the fluidic backplane • IP20, as standalone product |
| Directives | |
| CE directives | The applied standards, which verify conformity with the EU Directives, can be found on the EU Type Examination Certificate and/or the EU Declaration of conformity (if applicable). |
| Environment and installation | |
| Ambient temperature | |
| Operating | +3...+40 °C (+37...+104 °F) |
| Storage and transport | For empty/purged sensor cube: -10...+60 °C (+14...+140 °F) |
| Relative air humidity | ≤90 %, without condensation |
| Height above sea level | Max. 2000 m |
| Operating condition | Continuous |
| Equipment mobility | Fixed |
| Application range | Indoor and outdoor (Protect the device against electromagnetic interference, ultraviolet rays and, when installed outdoors, against the effects of climatic conditions) |
| Installation category | Category I according to UL/EN 61010-1 |
| Pollution degree | Degree 2 according to UL/EN 61010-1 |

2. Materials

2.1. Chemical Resistance Chart – Bürkert resistApp

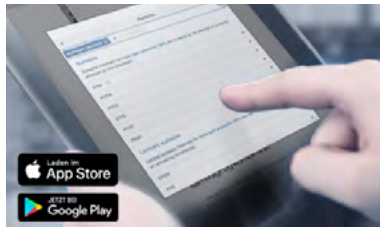

Bürkert resistApp – Chemical Resistance Chart


You want to ensure the reliability and durability of the materials in your individual application case? Verify your combination of media and materials on our website or in our resistApp.

[Start Chemical Resistance Check](#)

3. Dimensions

Note:

Dimensions in mm

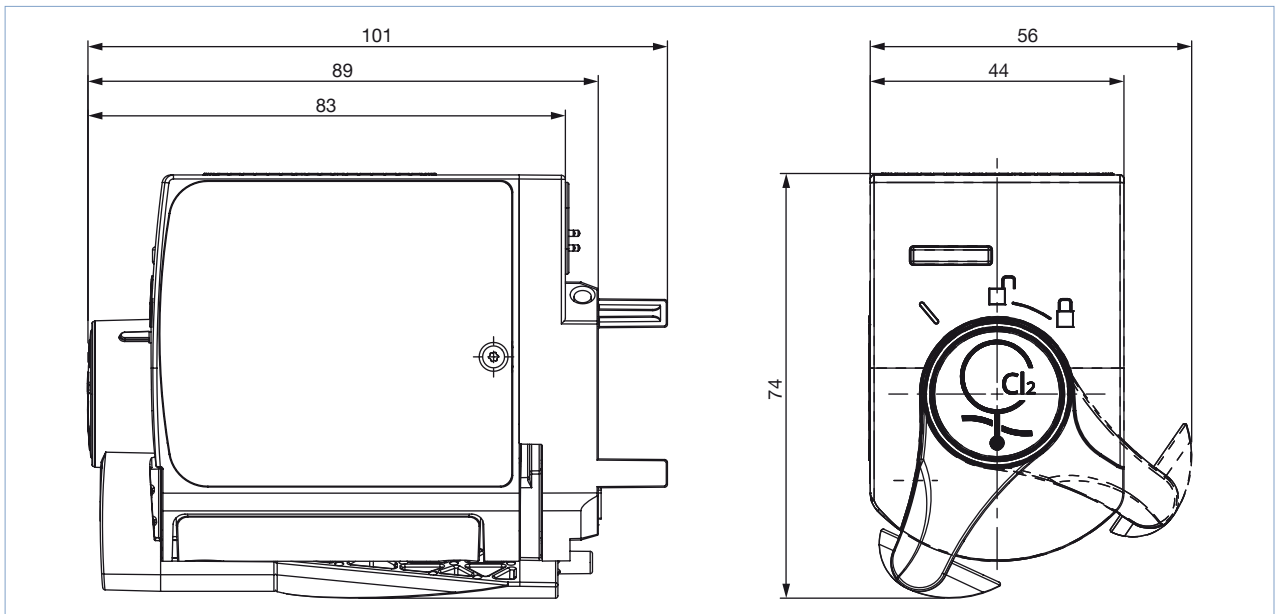

4. Product installation

4.1. Installation notes

Note:

- The sensor cube is designed for use with the online analysis system, Type 8905. The sensor cube is simply plugged into the backplane in Type 8905.
- It is also possible to mount the backplane individually on a DIN rail.

See **data sheet Type 8905** ▶ Online Analysis System for more information.


Installation examples

Product mounted in a housing for the Online analysis system Type 8905.

- Chlorine or chlorine dioxide sensor cube Type MS02
- Housing Type 8905 with display Type ME21 and controller Type ME25




Product without housing mounted on the backplane on standard rail (TS35).

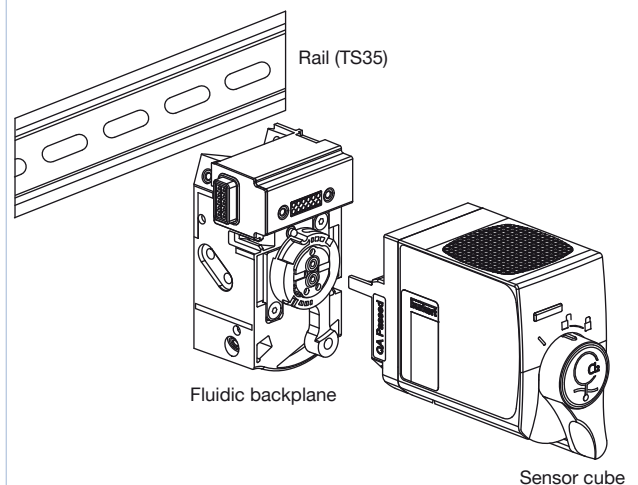

5. Product design and assembly

5.1. Product features

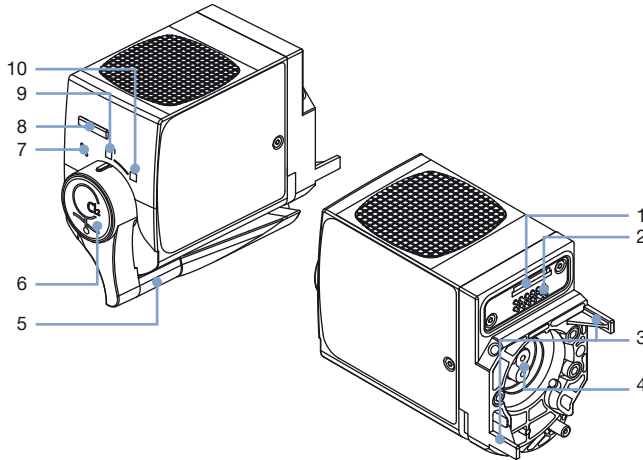

Product without housing

| No. | Element |
|-----|---|
| 1 | Slot micro-SIM card (for configuration data) |
| 2 | Electrical interface |
| 3 | Guide pins |
| 4 | Fluid connections |
| 5 | Lever to: <ul style="list-style-type: none"> lock / unlock the product carry out maintenance operations |
| 6 | Push button for unlocking |
| 7 | Maintenance position |
| 8 | Sensor cube Status LED |
| 9 | Unlocked position |
| 10 | Locked position |

6. Ordering information

6.1. Bürkert eShop – Easy ordering and quick delivery



Bürkert eShop – Easy ordering and fast delivery

You want to find your desired Bürkert product or spare part quickly and order directly? Our online shop is available for you 24/7. Sign up and enjoy all the benefits.

[Order online now](#)

6.2. Bürkert product filter



Bürkert product filter – Get quickly to the right product

You want to select products comfortably based on your technical requirements? Use the Bürkert product filter and find suitable articles for your application quickly and easily.

[Try out our product filter](#)

6.3. Ordering chart




Note:

The chlorine/chlorine dioxide sensor cube must be operated within a system.

Please refer to the order information for Online Analysis System Type 8905, see **data sheet Type 8905** ▶ or contact your Bürkert representative.

| Description | Article no. |
|--|--|
| Chlorine (Cl ₂) sensor cube | 567631  |
| Chlorine dioxyde (ClO ₂) sensor cube | 567722  |

6.4. Ordering chart accessories

| Description | Article no. |
|--|--|
| Photometer MD100, measuring range 0.01...6 ppm | 566393  |
| DPD-1 reagent (100 Tablets) | 566394  |
| Replacement part set: measurement cell | 568040  |

Bürkert – Close to You

For up-to-date addresses
please visit us at
www.burkert.com

DTS 1000220807 EN Version: J Status: RL (released | freigegeben | validé) printed: 20.12.2019

